


**Docket #:** S19-098

# **Quality Assurance (QA) Phantom for off-axis spatial accuracy for frameless single-isocenter Multitarget Stereotactic Radiosurgery**

Stanford researchers have developed and validated a quality assurance (QA) phantom that will facilitate the translation of a frameless volumetric modulated arc therapy radiosurgery technique. This is critically needed for the commissioning of linear accelerators to perform frameless single-isocenter multitarget stereotactic radiosurgery (SRS) and will enable clinical translation of this highly sought-after workflow solution.

This phantom provides the unique advantage of quantifying the spatial accuracy of a linear accelerator as a function of distance from isocenter (i.e. off-axis spatial accuracy/Winston-Lutz test), as well as the ability to perform various positioning systems acceptance tests and quantifying dosimetric accuracy. This invention will address one of the main bottlenecks limiting the implementation of a frameless single-isocenter, multitarget SRS program, improving efficiency without compromising on coverage or dose-delivery.

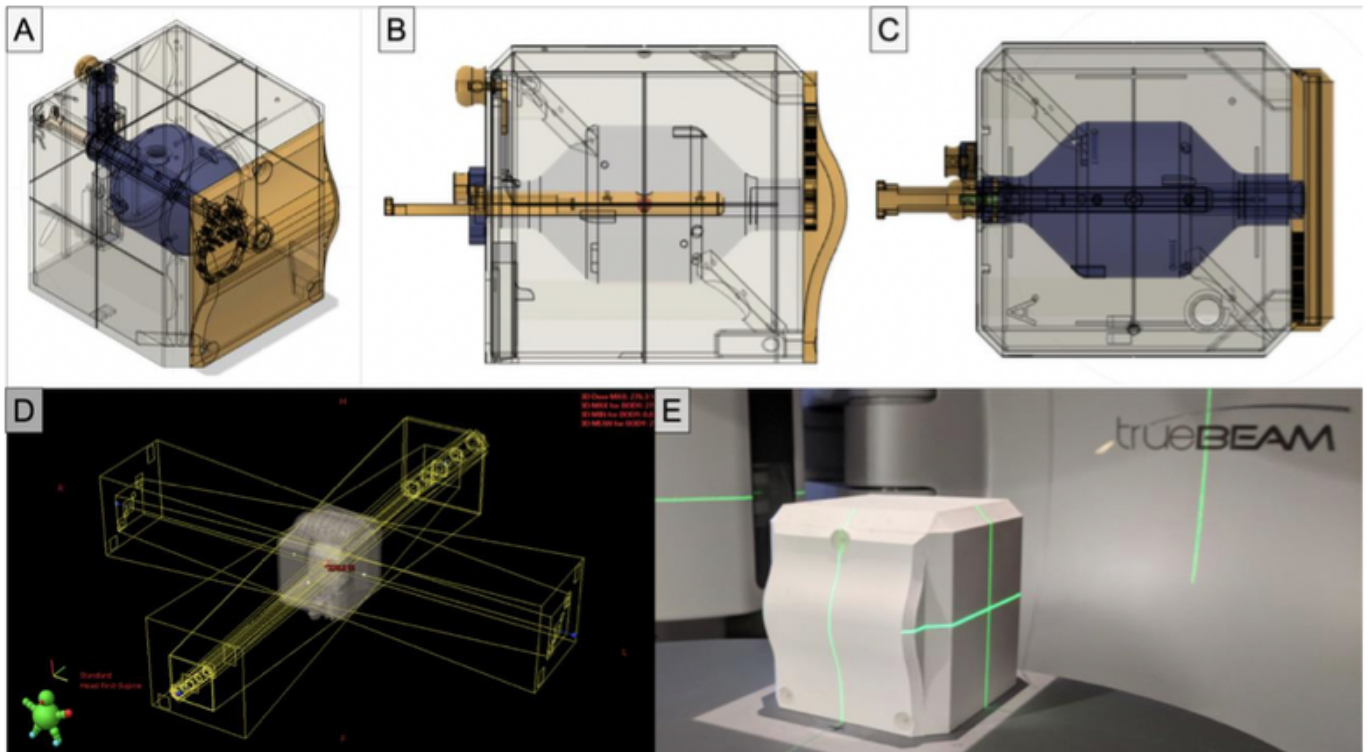

Design and development of a QA phantom to quantify the spatial accuracy of a linear accelerator- based single-isocenter, multitarget cranial radiosurgery system ( **A-C**). (**D**) Eclipse treatment plan portal fields. (**E**) 3D printed QA phantom on Varian Truebeam (Varian Medical Systems, Palo Alto, CA).

### **Stage of Research:**

**Prototype** phantom that has been used to acquire preliminary results

### **Related Technologies:**

US Patent Application US20190175951A1 ["Novel integrated multi-modal phantom for combined dosimetry and positioning verification"](#)

Stanford docket S17-451 ["A novel integrated quality assurance phantom for radiographic and non-radiographic radiotherapy localization and positioning systems"](#)

Stanford docket S19-067 ["Non-toxic 3D printed device for improving precision in electron beam radiotherapy"](#)

## **Applications**

- **Radiation oncology**, specifically for Brain SRS

## **Advantages**

- Uniquely capable of doing off-axis accuracy (off-axis Winston-Lutz) test - no other phantom can achieve this
- Facilitates translation of multitarget frameless VMAT radiosurgery technique
- Improves efficiency with lower overall treatment times
- Can QA surface image-guidance systems for frameless treatments which provide greater patient comfort with an open-faced mask and fast treatment times.

## **Innovators**

- Shu-Jung YU
- Lawrie Skinner
- Piotr Dubrowski
- Dante Capaldi

## **Licensing Contact**

### **Evan Elder**

Senior Licensing Associate

[Email](#)