

LINAC-Compatible Robotic Ultrasound Manipulator for Radiotherapy Guidance

Stanford researchers have developed a patented imaging probe manipulator that consistently maintains probe-to-patient contact pressure and compensates for patient respiratory motion and anatomy shifts during External Beam Radiation Therapy (EBRT). The non-invasive, marker-less, real time image guidance system delivers precise radiation doses to internal moving targets while sparing surrounding healthy structures. The system is lower cost than conventional x-ray based guided systems, can be integrated with any existing radiation delivery system and as an image guidance tool for biopsies, surgeries, and other procedures.

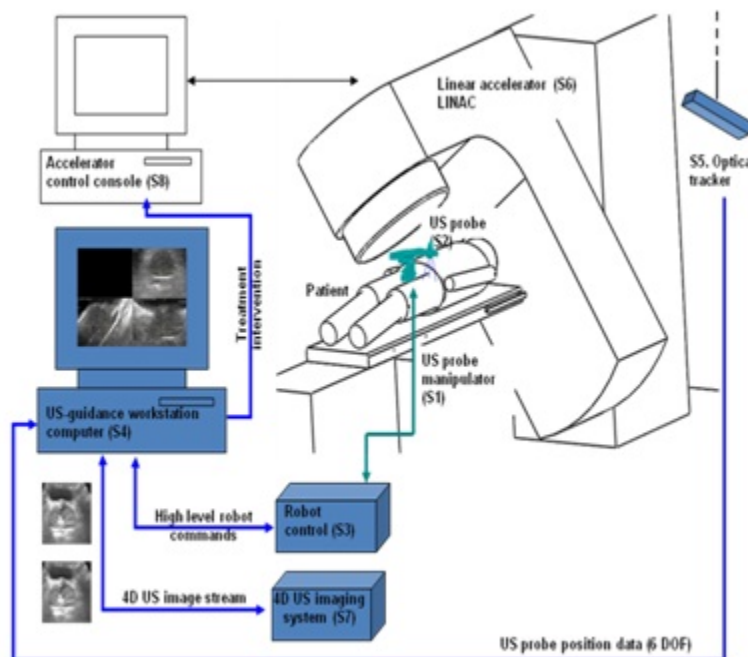


Figure 1 - Robotic ultrasound image guidance system in radiation therapy
(Image courtesy the Hristov Lab and Salisbury Robotics Lab)

Stage of Development - Prototype

Researchers demonstrated real-time, volumetric soft-tissue guidance during live radiotherapy delivery, with clinical viability confirmed through treatment planning analysis and seamless LINAC integration. Sub-3mm displacement detection aligns with clinical action thresholds in prostate radiotherapy, suggesting strong translational potential.

Applications

- **Radiation treatment:** Gantry-based radiotherapy, tomotherapy, Cyberknife radiotherapy
- **Trans-abdominal imaging** during radiation treatment
- Structure imaging such as skull, spine, etc.
- Hands-free image guidance tool for procedures such as **image guided biopsy, surgery, brachytherapy, needle insertion, catheter placement**, etc.

Advantages

- **Real-time** volumetric intra- and inter-fractional motion management based on soft-tissue 3D images
- **Non-invasive and markerless** - No use of ionizing radiation or need for implanted fiducial markers
- Compatible with existing radiation delivery platforms such as conventional C-arm LINAC as well as with Cyberknife radiosurgery robot or tomotherapy systems
- Compatible with existing radiotherapy workflows as an add-on device
- **Lower cost** than conventional x-ray-based guidance systems

Publications

- Schlosser, J., Salisbury, K., & Hristov, D. (2012). [Online image-based monitoring of soft-tissue displacements for radiation therapy of the prostate](https://doi.org/10.1016/j.ijrobp.2011.10.049). *International Journal of Radiation Oncology* Biology* Physics*, 83(5), 1633-1640.
<https://doi.org/10.1016/j.ijrobp.2011.10.049>

- Schlosser, J., Salisbury, K., & Hristov, D. (2010). [Telerobotic system concept for real-time soft-tissue imaging during radiotherapy beam delivery](#). *Medical physics*, 37(12), 6357-6367. <https://doi.org/10.1118/1.3515457>

Patents

- Published Application: [WO2014018983](#)
- Published Application: [20150209599](#)
- Issued: [10,232,194 \(USA\)](#)

Innovators

- Jeffrey Schlosser
- Dimitre Hristov
- J. Kenneth Salisbury Jr.

Licensing Contact

Evan Elder

Associate Director, Licensing and Strategic Alliances, Physica

[Email](#)